


OCT. 1969 HSP
 FEB. 1970 G.G.
 AUG. 1970 G.G.

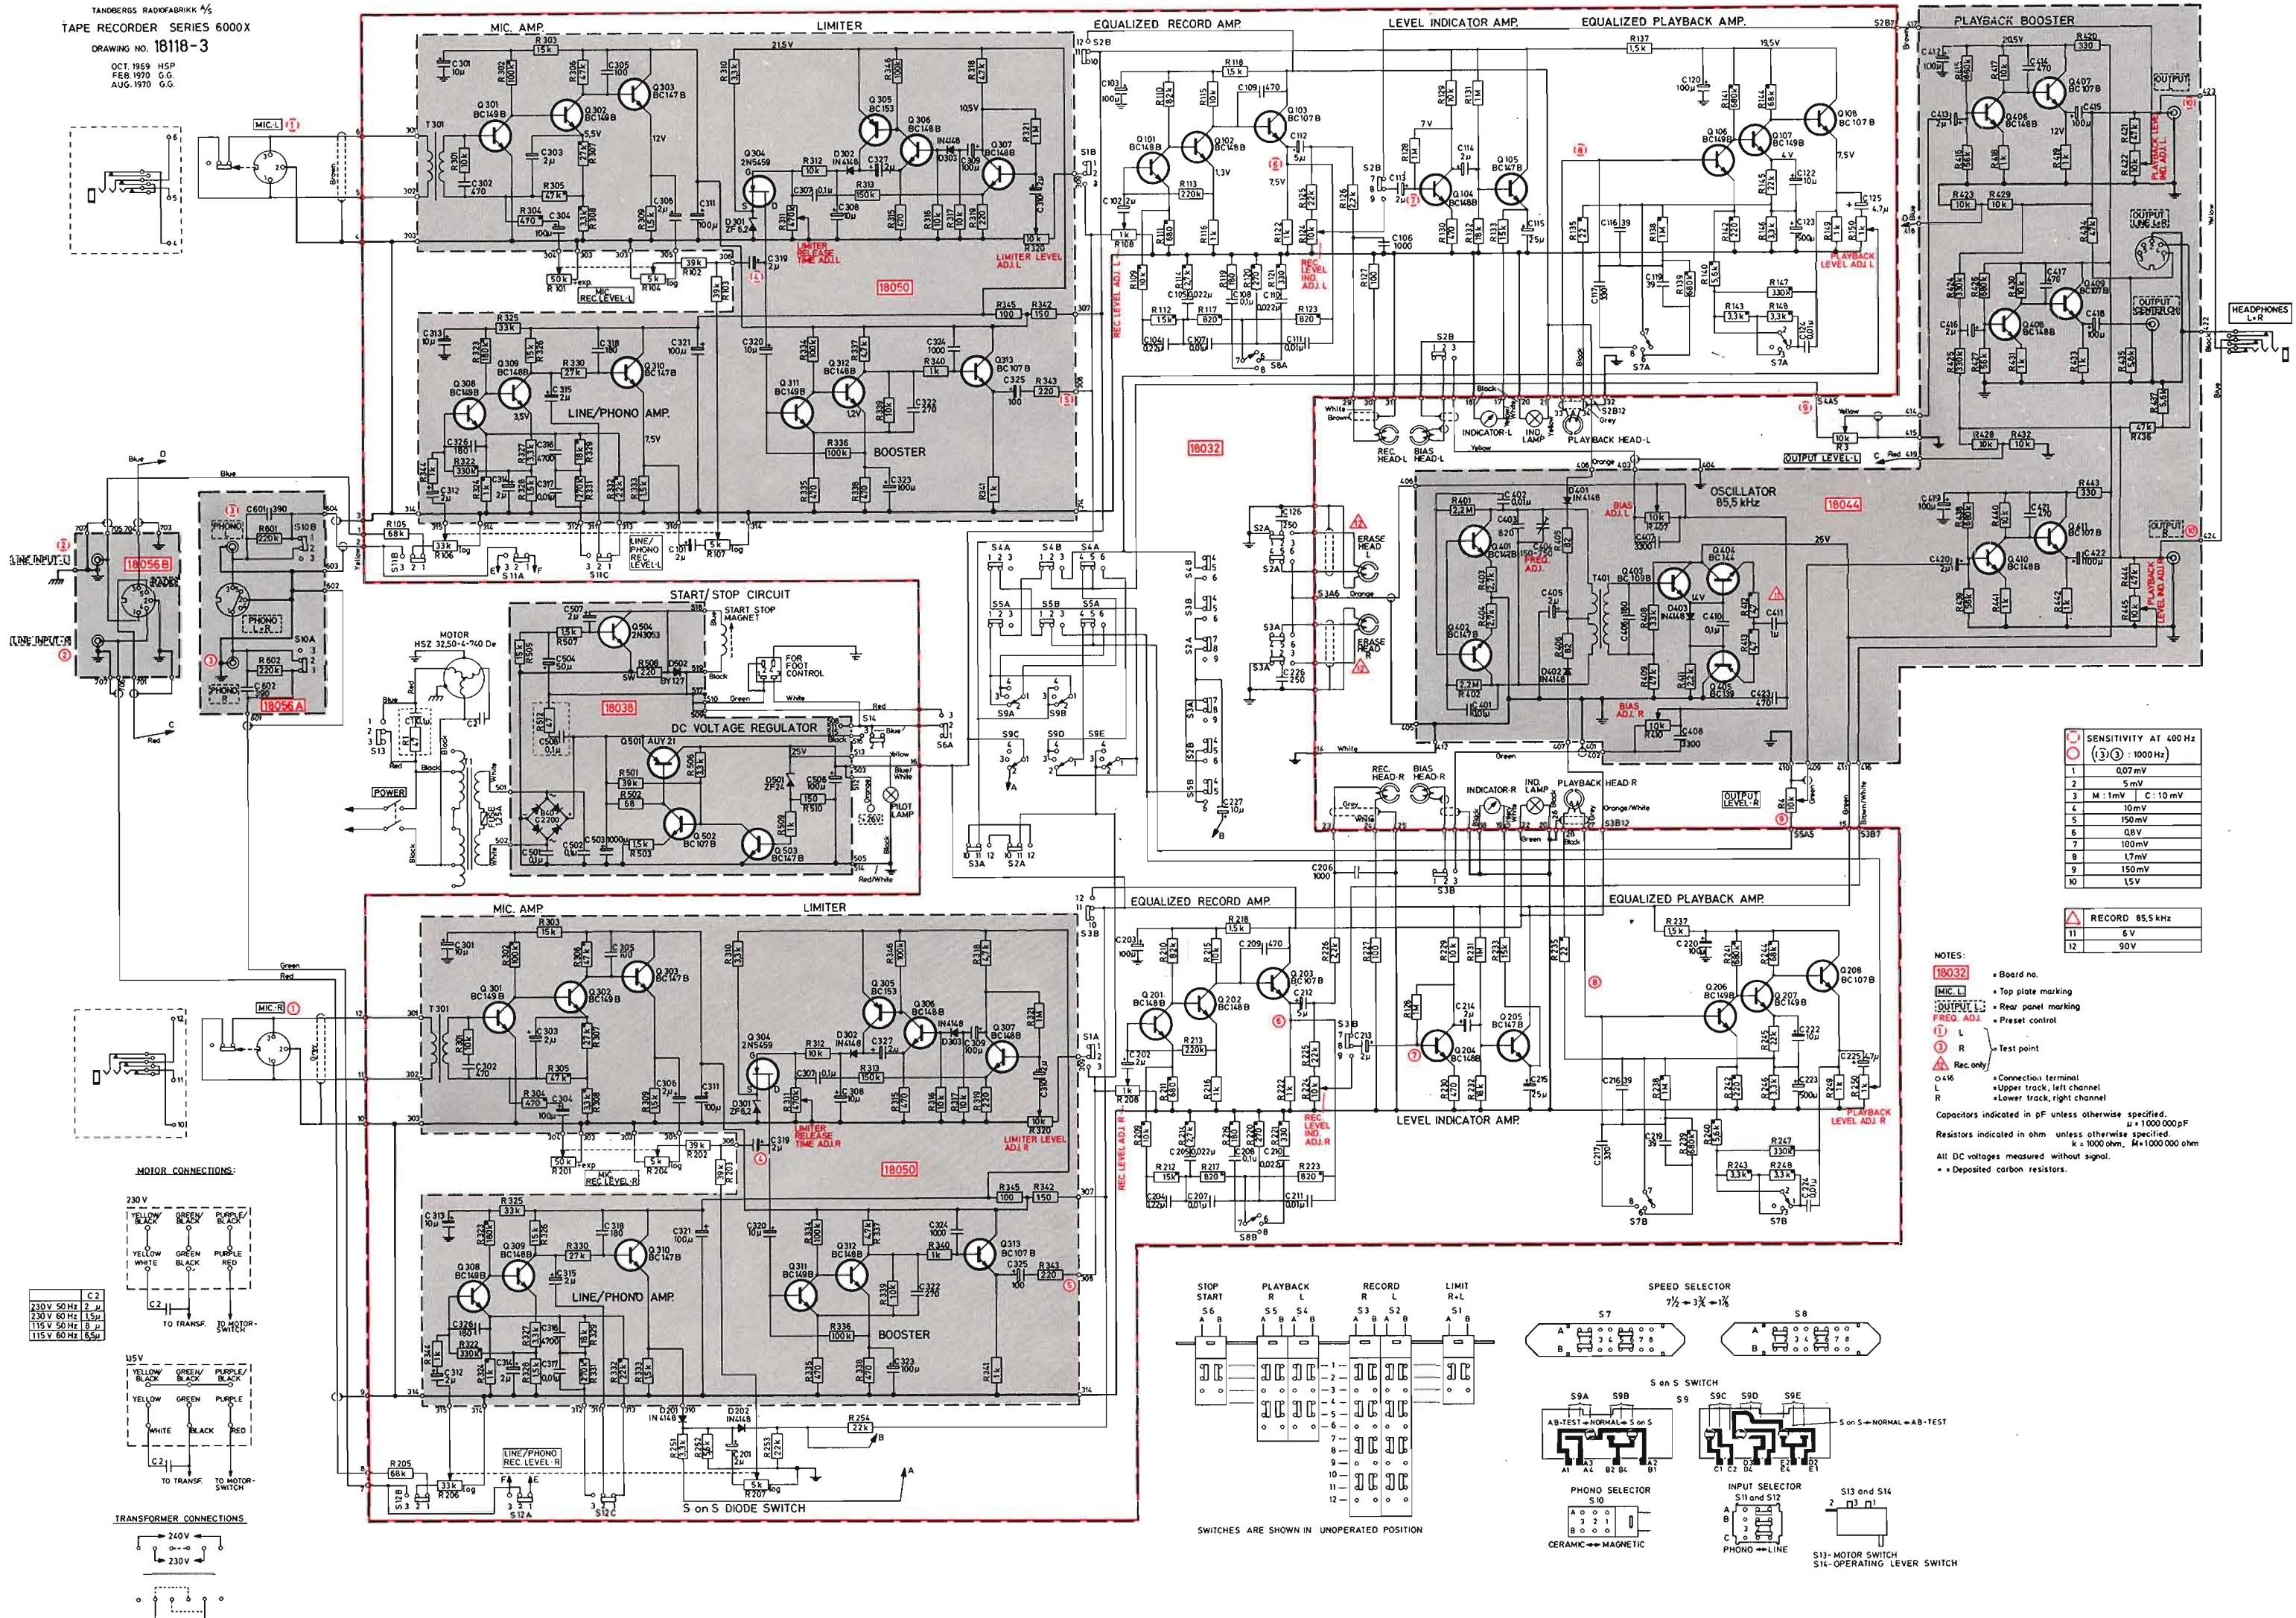

SENSITIVITY AT 400 Hz
 (3) (3) 1000 Hz

1	0.07 mV
2	5 mV
3	M: 1 mV C: 10 mV
4	10 mV
5	150 mV
6	0.8V
7	100 mV
8	1.7 mV
9	150 mV
10	1.5V

RECORD 85.5 kHz

11	5V
12	90V

NOTES:

- 18032 = Board no.
- MIC L = Top plate marking
- OUTPUT L = Rear panel marking
- FREQ. ADJ. = Preset control
- (1) L = Test point
- (2) R = Test point
- Rec. only
- o 46 = Connection terminal
- L = Upper track, left channel
- R = Lower track, right channel

Capacitors indicated in pF unless otherwise specified.
 Resistors indicated in ohm unless otherwise specified.
 k = 1000 ohm, M = 1000000 ohm
 All DC voltages measured without signal.
 * = Deposited carbon resistors.

